STOP! READ FIRST!

IMPORTANT: DONORS SHOULD NOT PLACE ANYTHING (INCLUDING FOOD, DRINK, GUM OR TOBACCO PRODUCTS) IN THEIR MOUTH FOR AT LEAST 10 MINUTES PRIOR TO THE PROCEDURE. DO NOT BITE, SUCK, OR CHEW ON THE SPONGE. REFRAIN FROM TALKING WHILE COLLECTION SWAB IS IN THE MOUTH.



Follow these instructions for the best results with this innovative screening device, which includes market-leading drug cutoffs and the first-ever sponge saturation indicator.

The purpose of Step 1 is to saturate the sponge with saliva. With collection swab (B), have donor sweep the inside of mouth (cheek, gums, tongue) several times, then hold swab in closed mouth until color on the saturation indicator strip appears in the indicator window.

Donor must leave swab in mouth until instructed to remove it. Donor may remove swab from mouth when color appears in the indicator window.

Note: If at 7 minutes, color on saturation indicator has not appeared in indicator window, proceed with test (Step 2).



Remove collection swab from mouth and insert sponge first into screening device (A), pushing until the locking flange locks in place in the bottom of device. Once locked in place, the device

is airtight, tamper evident, and ready to dispose of after use or send to lab for confirmation (on presumptive positive result). Ensure that specimen is contacting all test strips. If not, rotate the device side to side / front to back to disperse the specimen within the chamber.





EXAMPLE: 45° maximum rotation


Services Services

Services Serv

With specimen dispersed, set device upright on flat surface. Keep upright while test is running.

3

Read negative results as soon as two lines appear on any test strip, often within 2 minutes. Any indication of a line in the test region (T) should be considered a line, and therefore a negative result. Read presumptive positive results at 10 minutes.




EXAMPLE: Presumptive positive for cocaine (COC)




Note: The THC (marijuana) strip has improved sensitivity, which may show a less intense color band in the test region (T). This is an expected and normal response.

If the device includes alcohol, read the alcohol strip at 2 minutes. Compare the color of the reaction pad with the color chart provided to determine the relative blood alcohol level. No color change indicates a negative result.





Cut out this panel to copy or scan results

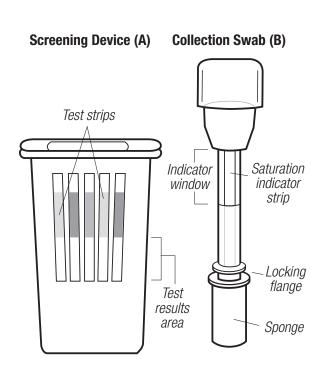

TEST RESULTS RECORD

Test Reference Number		Name of Collector						
COMPANY INF	ORMATION							
Company Name			Phone		Fax			
Address	City			State/Province		Zip/Postal Code		
DONOR INFOR	MATION		Employee I D					
Last Name								
Type of Identification Provided: Driver's License Employee Photo I.I.								
Reason for test: Pre-e	mployment 🔲 Randon	Reasonable cause	Post-accident	Other				
CERTIFICATION	V							
I hereby certify that the spec			d or adulterated. I furth	ner agree and gr	ant			
permission for the testing of	r my specimen for arug me	tadolites and alconol.						
Donor signature	ate / Time		-					
I hereby certify that I collect adulterated to the best of m		by the aforementioned Dono	r and that it was not s	ubstituted or				
					-			
Collector signature		U	ate / Time					
Laboratory signature			ate / Time received		-			
TEST RESULTS			Drug N	lama	Symbol	Negative	Positive	Not Tested
ILOI IILOULIO	,		Alcohol	iaiiie	ALC			
Date/Time Collected			Amphetam	nine	AMP	_	_	_
Time Interpreted			Buprenorp		BUP			
			Benzodiaz	epine	BZ0			
NOTE: Lab personnel obtain		ide of Device	Cocaine		COC			
by puncturing the lab extraction ports on the side of device with a needle and syringe and drawing out the sample.		1	EDDP		EDDP			
			Marijuana		THC			
			Methadon		MTD			
			Methamph	netamine	MET			
			Opiates		OPI			
	lo	< LAB EXTRACTION PORTS >	Oxycodone		OXY			
Out and this manual to			Phencyclic	line	PCP			
Cut out this panel to copy or scan results	<u>L</u>	ab extraction ports						
	Notes / Comments							
	140103 / OUIIIIIIGIIIS _							